

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 510 021

Grad. pipettes, 0,2:0,01 ml, AS, conf. cert.




Batch: 48-20

Serial:

Measuring Nr. 43220

Batch size: 275

Volume:	0,2000 ml	0,1200 ml	0,0400 ml
Tolerance:	± 0,0060 ml	± 0,0060 ml	± 0,0060 ml
Average value:	0,2000 ml	0,1207 ml	0,0394 ml
Deviation:	0,0013 ml	0,0015 ml	0,0005 ml
Precision (CV):	0,6660 %	1,2517 %	1,3057 %

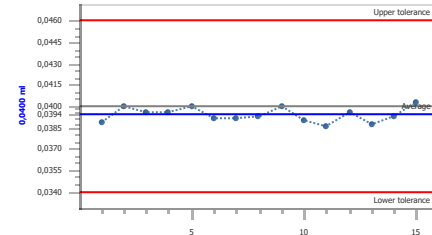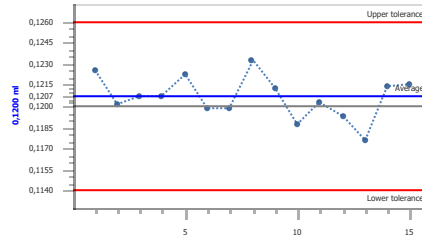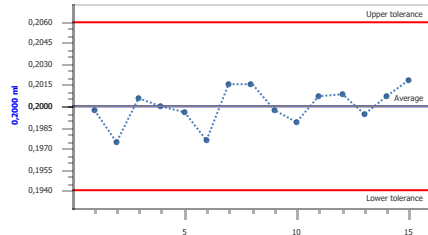

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 835

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	7
Date:	11.12.2020
Balance:	Sartorius - LE244S-OCE

