

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 510 051 BL

Grad. pipettes, 0,5:0,01 ml, blue grad., AS, conf. cert.




Batch: 13-18

Serial:

Measuring Nr. 19525

Batch size: 500

Volume:	0,5000 ml	0,3000 ml	0,1000 ml
Tolerance:	± 0,0060 ml	± 0,0060 ml	± 0,0060 ml
Average value:	0,5002 ml	0,2997 ml	0,0989 ml
Deviation:	0,0014 ml	0,0008 ml	0,0003 ml
Precision (CV):	0,2857 %	0,2651 %	0,3388 %

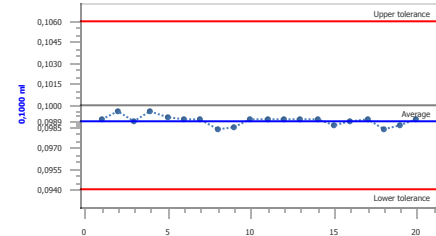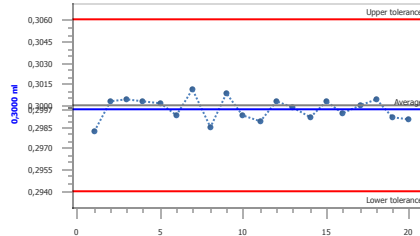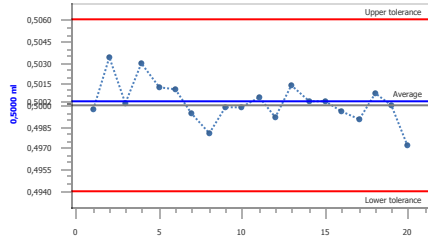

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 835

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	44
Date:	06.04.2018
Balance:	Sartorius - LE244S-OCE

