

# Certificate of performance



ISO 9001  
CERTIFIED

**Article:** 3 510 051

**Graduated pipettes, 0,5:0,01 ml, AS, conf. cert.**




**Batch:** 45-19

**Serial:**

**Measuring Nr.** 34371

**Batch size:** 435

Volume:	0,5000 ml	0,3000 ml	0,1000 ml
<b>Tolerance:</b>	± 0,0060 ml	± 0,0060 ml	± 0,0060 ml
<b>Average value:</b>	0,4979 ml	0,3014 ml	0,1004 ml
<b>Deviation:</b>	0,0011 ml	0,0013 ml	0,0010 ml
<b>Precision (CV):</b>	0,2242 %	0,4186 %	0,9510 %

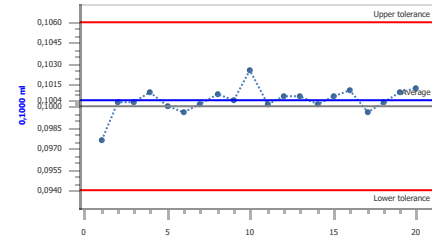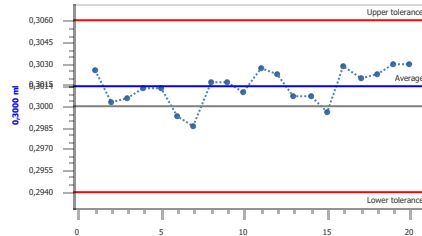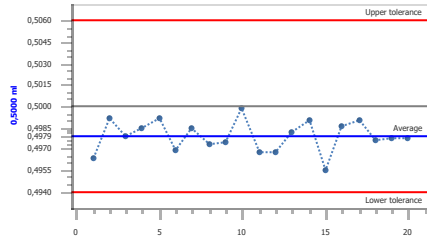

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 835

**witeg Labortechnik GmbH**

Am Bildacker 16  
97877 Wertheim  
Germany  
+49 (0) 9342 / 9301-0  
info@witeg.de

<b>Operator:</b>	7
<b>Date:</b>	12.11.2019
<b>Balance:</b>	Sartorius - MSE224S-0CE -DU

DE-M