

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 510 101 USP

Grad. pipettes, 1:0,01 ml, AS, USP, conf. cert.




Batch: 23-20

Serial:

Measuring Nr. 38568

Batch size: 90

Volume:	1,0000 ml	0,6000 ml	0,2000 ml
Tolerance:	± 0,0070 ml	± 0,0070 ml	± 0,0070 ml
Average value:	0,9992 ml	0,5976 ml	0,1996 ml
Deviation:	0,0018 ml	0,0016 ml	0,0005 ml
Precision (CV):	0,1802 %	0,2655 %	0,2660 %

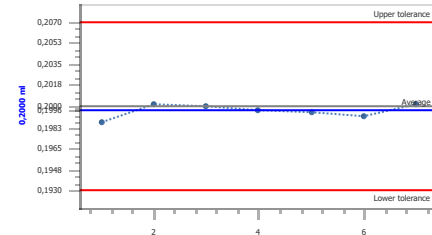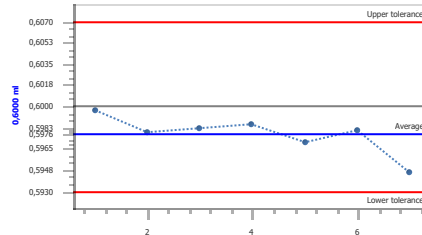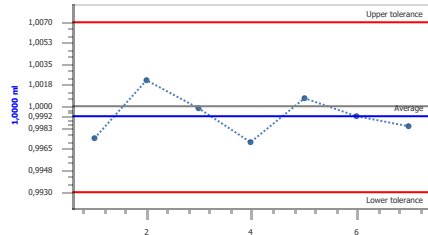

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 835

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	9
Date:	10.06.2020
Balance:	Sartorius - LE244S-OCE

DE-M