

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 510 110

Grad. pipettes, 1:0,1 ml, AS, conf. cert.




Batch: 46-21

Serial:

Measuring Nr. 50913

Batch size: 270

Volume:	1,0000 ml	0,6000 ml	0,2000 ml
Tolerance:	± 0,0070 ml	± 0,0070 ml	± 0,0070 ml
Average value:	0,9997 ml	0,6012 ml	0,2006 ml
Deviation:	0,0017 ml	0,0019 ml	0,0006 ml
Precision (CV):	0,1713 %	0,3224 %	0,3144 %

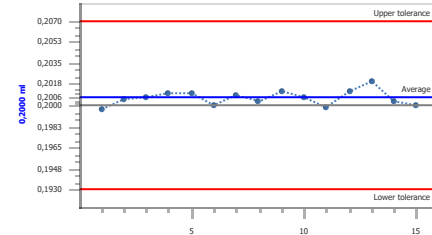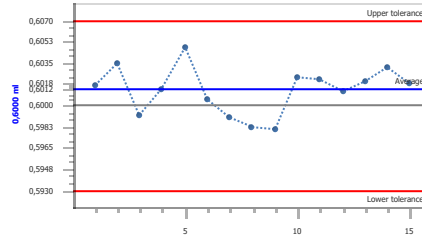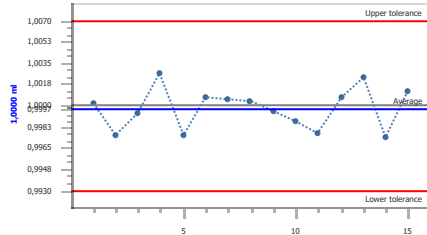

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 835

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	7
Date:	30.11.2021
Balance:	Sartorius - LE244S-OCE

