

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 510 210

Grad. pipettes, 2:0,1 ml, AS, conf. cert.




Batch: 23-20

Serial:

Measuring Nr. 38602

Batch size: 118

Volume:	2,0000 ml	1,2000 ml	0,4000 ml
Tolerance:	± 0,0100 ml	± 0,0100 ml	± 0,0100 ml
Average value:	1,9993 ml	1,2018 ml	0,4032 ml
Deviation:	0,0035 ml	0,0025 ml	0,0013 ml
Precision (CV):	0,1762 %	0,2106 %	0,3250 %

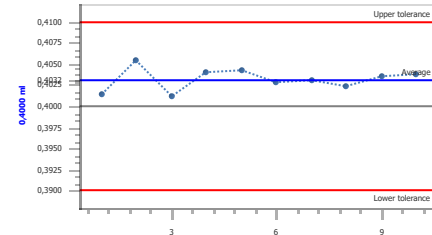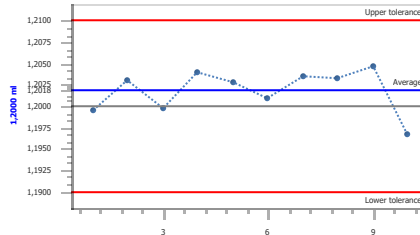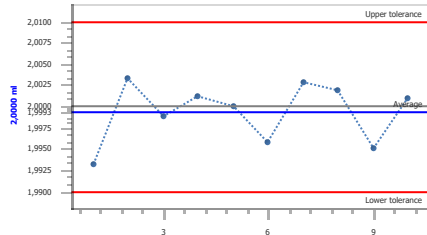

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 835

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	7
Date:	15.06.2020
Balance:	Sartorius - MSE224S-0CE -DU

