

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 510 210

Grad. pipettes, 2:0,1 ml, AS, conf. cert.

Batch: 41-20




Serial:

Measuring Nr. 41588

Batch size:

280

Volume:	2,0000 ml	1,2000 ml	0,4000 ml
Tolerance:	± 0,0100 ml	± 0,0100 ml	± 0,0100 ml
Average value:	1,9995 ml	1,2008 ml	0,4022 ml
Deviation:	0,0031 ml	0,0032 ml	0,0013 ml
Precision (CV):	0,1556 %	0,2662 %	0,3371 %

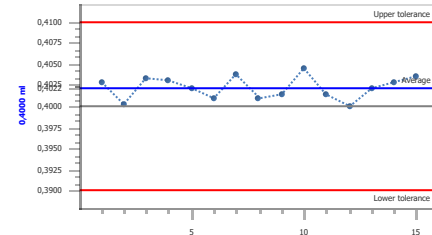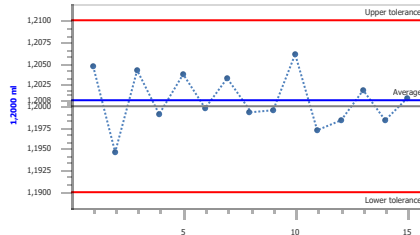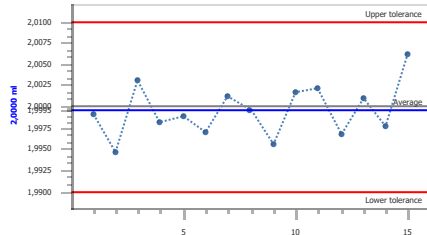

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 835

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:

7

Date:

20.10.2020

Balance:

Sartorius -
LE244S-0CE

DE-M