

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 510 505 USP

graduated pipettes 5 ml class AS USP KB

Batch: 20-21




Serial:

Measuring Nr.: 47068

Batch size:

280

Volume:	5,0000 ml	3,0000 ml	1,0000 ml
Tolerance:	± 0,0200 ml	± 0,0200 ml	± 0,0200 ml
Average value:	4,9974 ml	2,9907 ml	0,9986 ml
Deviation:	0,0047 ml	0,0037 ml	0,0019 ml
Precision (CV):	0,0940 %	0,1249 %	0,1863 %

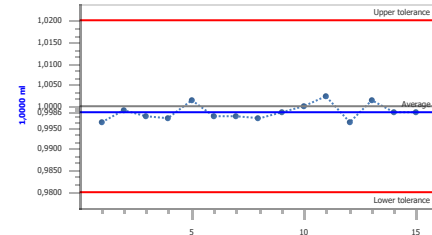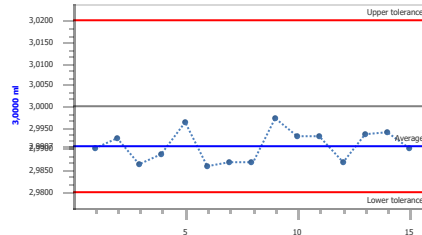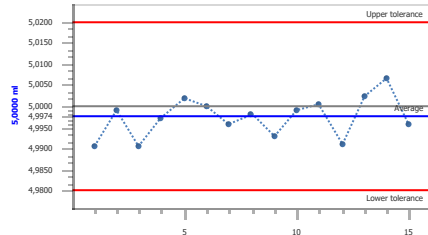

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 835

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	7
Date:	07.06.2021
Balance:	Sartorius - LE244S-OCE

