

# Certificate of performance



ISO 9001  
CERTIFIED

**Article:** 3 510 505

**Graduated pipettes, 5:0,5 ml, AS, conf. cert.**




**Batch:** 05-18

**Serial:**

**Measuring Nr.** 18279

**Batch size:** 3200

Volume:	5,0000 ml	3,0000 ml	1,0000 ml
Tolerance:	± 0,0300 ml	± 0,0300 ml	± 0,0300 ml
Average value:	4,9939 ml	2,9916 ml	0,9995 ml
Deviation:	0,0066 ml	0,0041 ml	0,0028 ml
Precision (CV):	0,1324 %	0,1361 %	0,2832 %

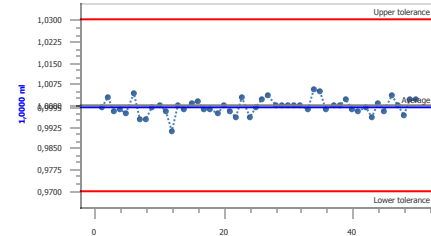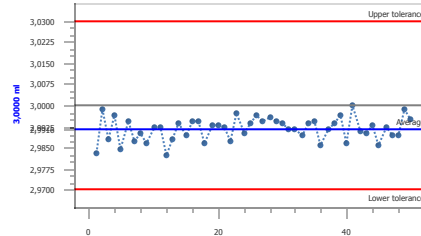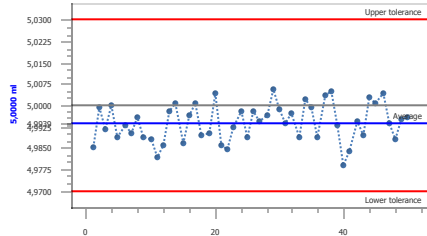

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 835

**witeg Labortechnik GmbH**

Am Bildacker 16  
97877 Wertheim  
Germany  
+49 (0) 9342 / 9301-0  
info@witeg.de

Operator:	9
Date:	21.02.2018
Balance:	Sartorius - LE244S-OCE

