

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 510 505

Graduated pipettes, 5:0,05 ml, AS, conf. cert.




Batch: 45-19

Serial:

Measuring Nr. 34401

Batch size: 5000

Volume:	5,0000 ml	3,0000 ml	1,0000 ml
Tolerance:	± 0,0300 ml	± 0,0300 ml	± 0,0300 ml
Average value:	4,9924 ml	2,9959 ml	1,0009 ml
Deviation:	0,0067 ml	0,0073 ml	0,0036 ml
Precision (CV):	0,1338 %	0,2442 %	0,3633 %

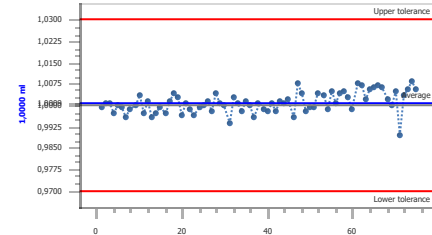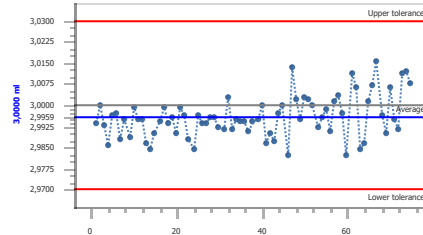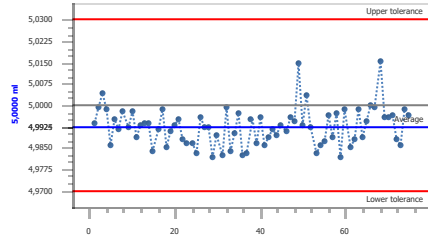

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 835

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	9
Date:	13.11.2019
Balance:	Sartorius - LE244S-OCE

