

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 510 505

Graduated pipettes, 5:0,05 ml, AS, conf. cert.




Batch: 21-20

Serial:

Measuring Nr. 38426

Batch size: 1993

Volume:	5,0000 ml	3,0000 ml	1,0000 ml
Tolerance:	± 0,0300 ml	± 0,0300 ml	± 0,0300 ml
Average value:	4,9932 ml	2,9970 ml	1,0010 ml
Deviation:	0,0066 ml	0,0056 ml	0,0032 ml
Precision (CV):	0,1311 %	0,1874 %	0,3213 %

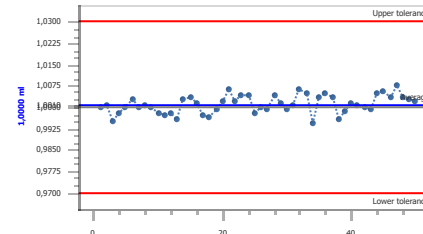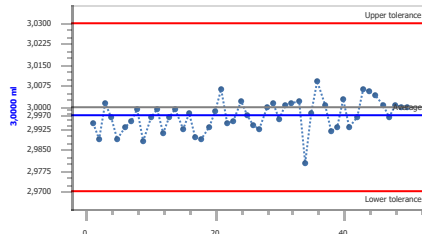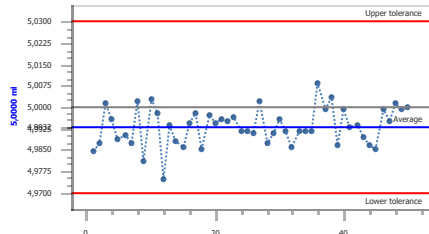

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 835

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	9
Date:	04.06.2020
Balance:	Sartorius - LE244S-OCE

DE-M