

Certificate of performance



Article: 3 510 505

Graduated pipettes, 5:0,05 ml, AS, conf. cert.




Batch: 50-23

Serial:

Measuring Nr. 65486

Batch size: 3200

Volume:	5,0000 ml	3,0000 ml	1,0000 ml
Tolerance:	± 0,0300 ml	± 0,0300 ml	± 0,0300 ml
Average value:	4,9865 ml	2,9906 ml	0,9978 ml
Deviation:	0,0057 ml	0,0046 ml	0,0027 ml
Precision (CV):	0,1148 %	0,1539 %	0,2700 %

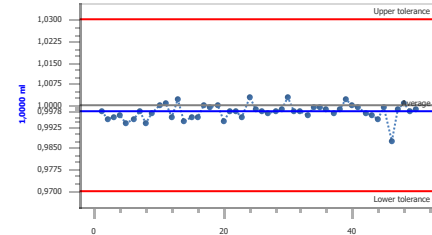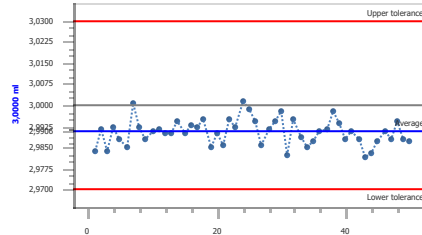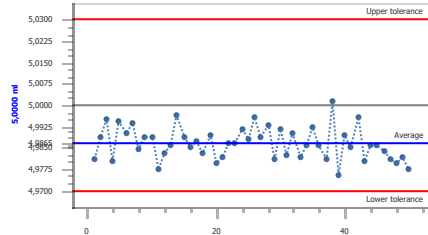

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 835

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	7
Date:	18.12.2023
Balance:	Sartorius - LE244S-OCE

