

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 510 510 BL

Grad. pipettes, 5:0,1 ml, blue grad., AS, conf. cert.




Batch: 28-21

Serial:

Measuring Nr. 48162

Batch size: 1197

Volume:	5,0000 ml	3,0000 ml	1,0000 ml
Tolerance:	± 0,0300 ml	± 0,0300 ml	± 0,0300 ml
Average value:	4,9962 ml	2,9977 ml	1,0020 ml
Deviation:	0,0048 ml	0,0050 ml	0,0032 ml
Precision (CV):	0,0963 %	0,1676 %	0,3152 %

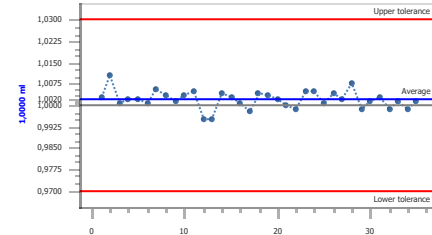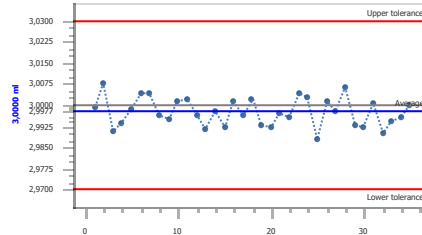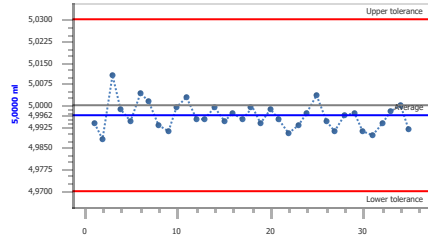

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 835

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	7
Date:	03.08.2021
Balance:	Sartorius - LE244S-OCE

