

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 510 510

Grad. pipettes, 5:0,1 ml, AS, conf. cert.




Batch: 51-17

Serial:

Measuring Nr. 17279

Batch size: 1200

Volume:	5,0000 ml	3,0000 ml	1,0000 ml
Tolerance:	± 0,0300 ml	± 0,0300 ml	± 0,0300 ml
Average value:	4,9912 ml	2,9958 ml	0,9990 ml
Deviation:	0,0055 ml	0,0076 ml	0,0033 ml
Precision (CV):	0,1108 %	0,2529 %	0,3305 %

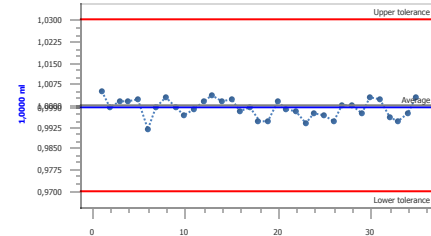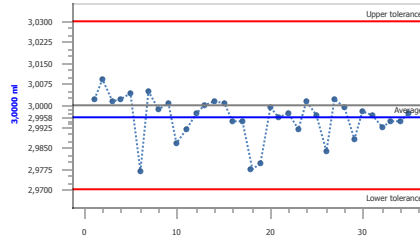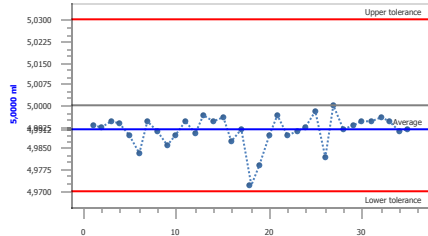

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 835

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	9
Date:	19.01.2018
Balance:	Sartorius - LE244S-OCE

