

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 510 710 BL

Grad. pipettes, 10:0,1 ml, blue grad., AS, conf. cert.




Batch: 35-17

Serial:

Measuring Nr. 13549

Batch size: 1200

Volume:	10,000 ml	6,0000 ml	2,0000 ml
Tolerance:	± 0,0500 ml	± 0,0500 ml	± 0,0500 ml
Average value:	9,9963 ml	5,9915 ml	1,9962 ml
Deviation:	0,0053 ml	0,0076 ml	0,0034 ml
Precision (CV):	0,0529 %	0,1262 %	0,1682 %

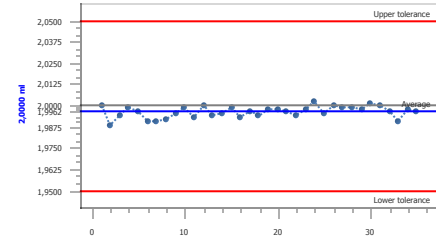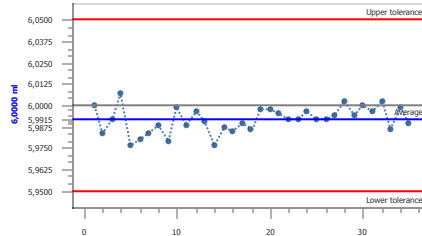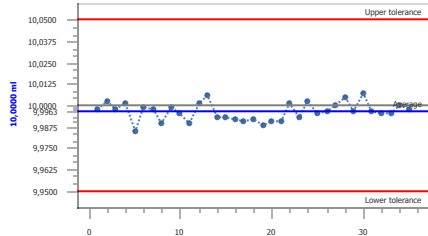

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 835

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	4
Date:	04.09.2017
Balance:	Sartorius - LE244S-OCE

