

# Certificate of performance



ISO 9001  
CERTIFIED

**Article:** 3 510 710 BL

**Grad. pipettes, 10:0,1 ml, blue grad., AS, conf. cert.**




**Batch:** 45-19

**Serial:**

**Measuring Nr.** 34232

**Batch size:** 1200

Volume:	10,0000 ml	6,0000 ml	2,0000 ml
<b>Tolerance:</b>	± 0,0500 ml	± 0,0500 ml	± 0,0500 ml
<b>Average value:</b>	9,9937 ml	6,0049 ml	2,0075 ml
<b>Deviation:</b>	0,0085 ml	0,0076 ml	0,0065 ml
<b>Precision (CV):</b>	0,0849 %	0,1270 %	0,3227 %

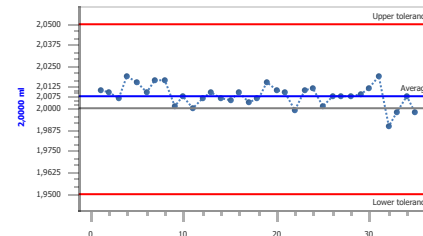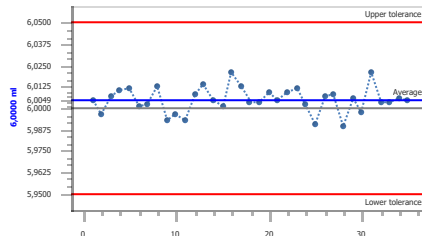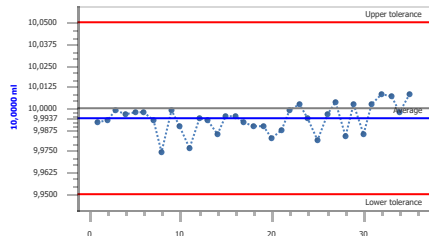

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 835

**witeg Labortechnik GmbH**

Am Bildacker 16  
97877 Wertheim  
Germany  
+49 (0) 9342 / 9301-0  
info@witeg.de

<b>Operator:</b>	9
<b>Date:</b>	07.11.2019
<b>Balance:</b>	Sartorius - LE244S-OCE

DE-M