

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 510 710 BL

Grad. pipettes, 10:0,1 ml, blue grad., AS, conf. cert.

Batch: 08-21




Serial:

Measuring Nr. 44642

Batch size:

500

Volume:	10,000 ml	6,0000 ml	2,0000 ml
Tolerance:	± 0,0500 ml	± 0,0500 ml	± 0,0500 ml
Average value:	9,9931 ml	5,9992 ml	1,9966 ml
Deviation:	0,0074 ml	0,0092 ml	0,0043 ml
Precision (CV):	0,0741 %	0,1537 %	0,2138 %

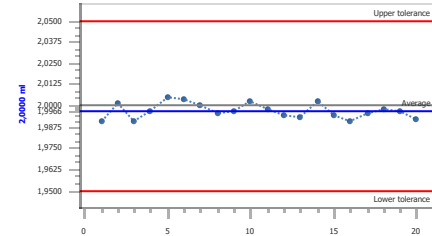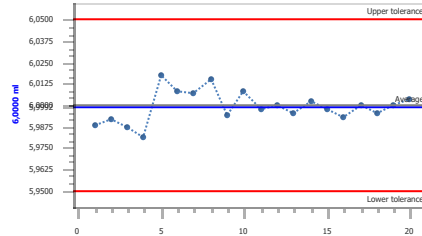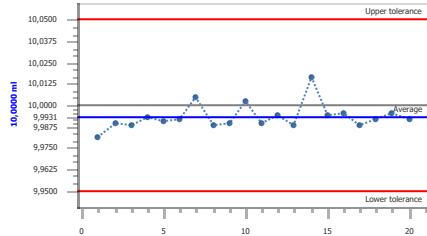

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 835

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:

7

Date:

24.02.2021

Balance:

Sartorius -
LE244S-OCE

DE-M