

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 510 710 USP

Graduated pipettes, 10:0,1 ml, USP, AS, conf.cert.




Batch: 09-21

Serial:

Measuring Nr. 44703

Batch size: 150

Volume:	10,000 ml	6,0000 ml	2,0000 ml
Tolerance:	± 0,0300 ml	± 0,0300 ml	± 0,0300 ml
Average value:	9,9995 ml	6,0012 ml	2,0063 ml
Deviation:	0,0066 ml	0,0087 ml	0,0057 ml
Precision (CV):	0,0660 %	0,1450 %	0,2848 %

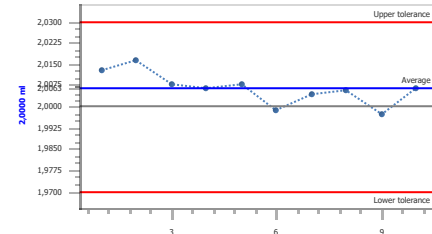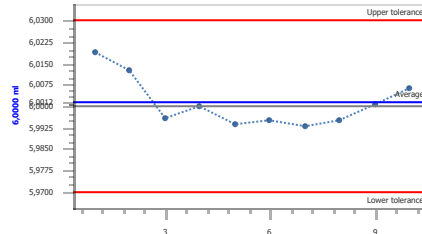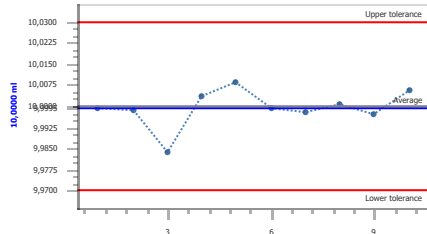

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 835

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	7
Date:	01.03.2021
Balance:	Sartorius - LE244S-OCE

