

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 510 710

Graduated pipettes, 10:0,1 ml, AS, conf. cert.




Batch: 02-20

Serial:

Measuring Nr. 35499

Batch size: 3200

Volume:	10,0000 ml	6,0000 ml	2,0000 ml
Tolerance:	± 0,0500 ml	± 0,0500 ml	± 0,0500 ml
Average value:	9,9921 ml	5,9956 ml	2,0052 ml
Deviation:	0,0085 ml	0,0132 ml	0,0068 ml
Precision (CV):	0,0855 %	0,2195 %	0,3406 %

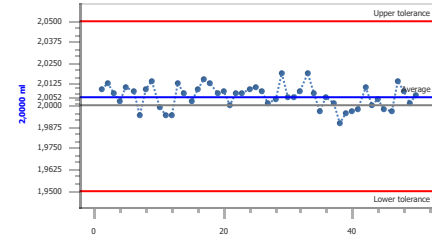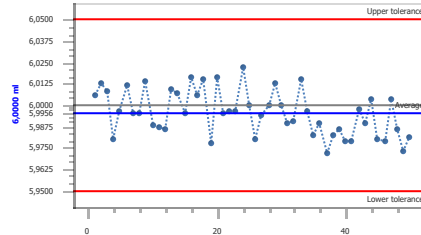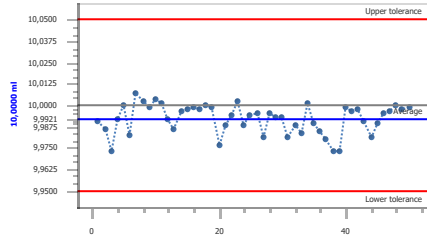

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 835

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	7
Date:	13.01.2020
Balance:	Sartorius - LE244S-OCE

