

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 510 810 BL

Grad. pipettes, 20:01, blue grad., AS, conf. cert




Batch: 07-21

Serial:

Measuring Nr. 44632

Batch size: 280

Volume:	20,000 ml	12,000 ml	4,000 ml
Tolerance:	± 0,1000 ml	± 0,1000 ml	± 0,1000 ml
Average value:	19,9945 ml	12,0169 ml	4,0090 ml
Deviation:	0,0131 ml	0,0129 ml	0,0061 ml
Precision (CV):	0,0655 %	0,1073 %	0,1523 %

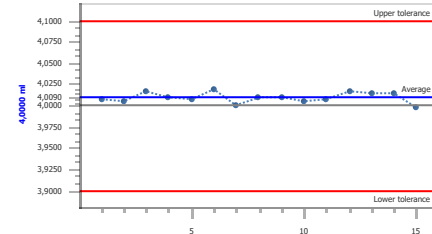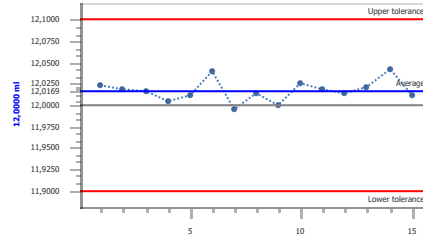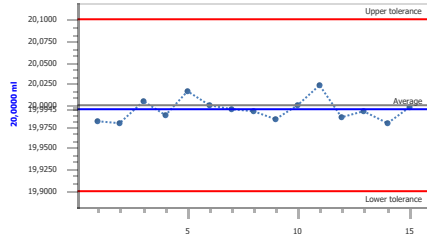

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 835

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	7
Date:	23.02.2021
Balance:	Sartorius - LE244S-OCE

