

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 510 810

Graduated pipettes, 20:0,1 ml, AS, conf. cert.

Batch: 18-21




Serial:

Measuring Nr. 46595

Batch size:

775

Volume:	20,000 ml	12,000 ml	4,000 ml
Tolerance:	± 0,1000 ml	± 0,1000 ml	± 0,1000 ml
Average value:	19,9885 ml	12,0207 ml	4,0164 ml
Deviation:	0,0157 ml	0,0233 ml	0,0083 ml
Precision (CV):	0,0783 %	0,1939 %	0,2087 %

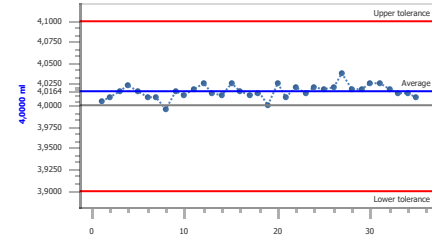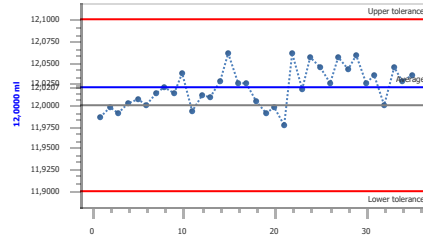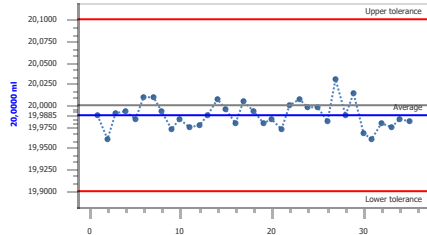

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 835

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:

7

Date:

11.05.2021

Balance:

Sartorius -
LE244S-OCE

DE-M