

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 510 910 BL

Grad. pipettes, 25:0,1 ml, blue grad., AS, conf. cert.




Batch: 49-18

Serial:

Measuring Nr. 26221

Batch size: 280

Volume:	25,000 ml	15,000 ml	5,000 ml
Tolerance:	± 0,1000 ml	± 0,1000 ml	± 0,1000 ml
Average value:	24,9905 ml	14,9972 ml	5,0006 ml
Deviation:	0,0078 ml	0,0159 ml	0,0096 ml
Precision (CV):	0,0310 %	0,1060 %	0,1924 %

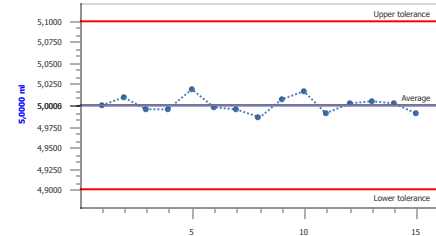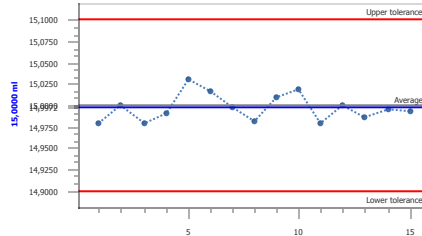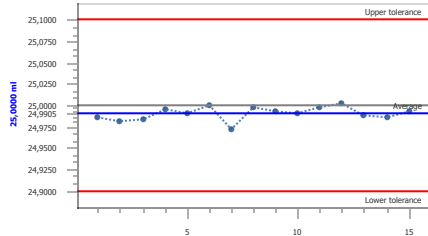

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 835

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	9
Date:	05.12.2018
Balance:	Sartorius - LE244S-OCE

