

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 510 910

Grad. pipettes, 25:0,1 ml, AS, conf. cert.




Batch: 05-23

Serial:

Measuring Nr. 61574

Batch size: 500

Volume:	25,0000 ml	15,0000 ml	5,0000 ml
Tolerance:	± 0,1000 ml	± 0,1000 ml	± 0,1000 ml
Average value:	24,9957 ml	14,9610 ml	4,9977 ml
Deviation:	0,0197 ml	0,0167 ml	0,0122 ml
Precision (CV):	0,0787 %	0,1116 %	0,2443 %

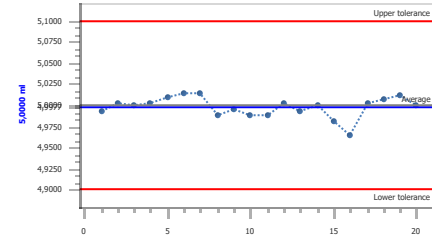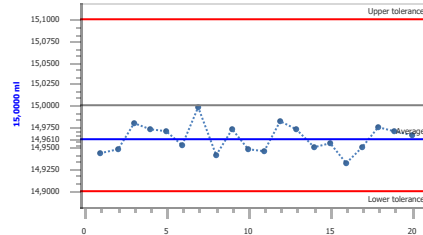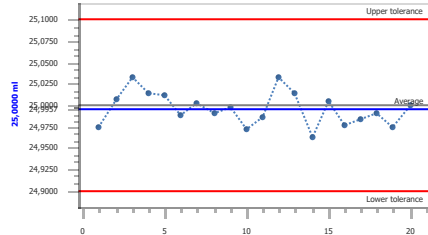

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 835

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	7
Date:	06.02.2023
Balance:	Sartorius - LE244S-OCE

