

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 515 101

Grad. pipette, 1 : 0,01 ml, AS, conf. cert.




Batch: 42-19

Serial:

Measuring Nr. 33730

Batch size: 651

Volume:	1,0000 ml	0,6000 ml	0,2000 ml
Tolerance:	± 0,0070 ml	± 0,0070 ml	± 0,0070 ml
Average value:	0,9998 ml	0,5996 ml	0,2003 ml
Deviation:	0,0023 ml	0,0021 ml	0,0012 ml
Precision (CV):	0,2296 %	0,3557 %	0,6071 %

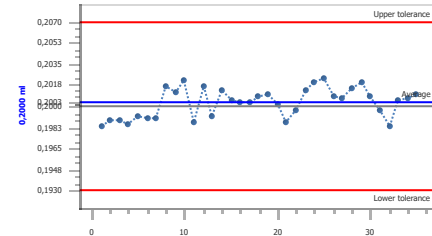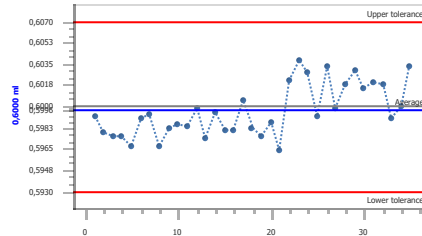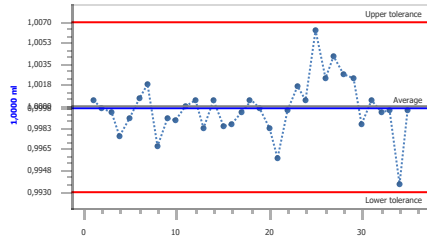

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 835

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	9
Date:	21.10.2019
Balance:	Sartorius - LE244S-OCE

DE-M