

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 515 110

Grad. pipette, 1:0,1 ml, AS, conf. cert.




Batch: 10-19

Serial:

Measuring Nr. 28269

Batch size: 150

Volume:	1,0000 ml	0,6000 ml	0,2000 ml
Tolerance:	± 0,0070 ml	± 0,0070 ml	± 0,0070 ml
Average value:	0,9989 ml	0,5982 ml	0,1996 ml
Deviation:	0,0025 ml	0,0014 ml	0,0009 ml
Precision (CV):	0,2494 %	0,2398 %	0,4590 %

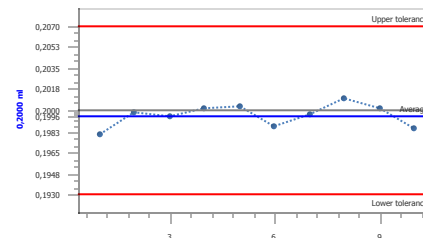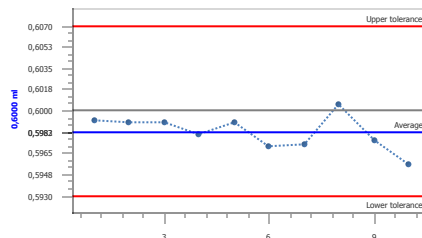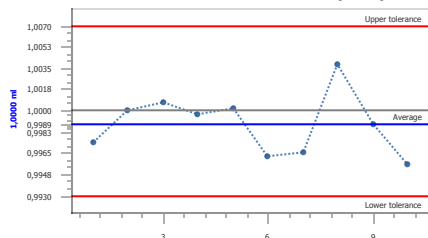

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 835

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	9
Date:	12.03.2019
Balance:	Sartorius - LE244S-OCE

DE-M