

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 515 202

Graduated pipette, 2:0,02 ml, AS, conf. cert.

Batch: 47-23




Serial:

Measuring Nr. 65359

Batch size:

280

Volume:	2,0000 ml	1,2000 ml	0,4000 ml
Tolerance:	± 0,0100 ml	± 0,0100 ml	± 0,0100 ml
Average value:	2,0000 ml	1,2022 ml	0,4022 ml
Deviation:	0,0022 ml	0,0025 ml	0,0014 ml
Precision (CV):	0,1107 %	0,2094 %	0,3611 %

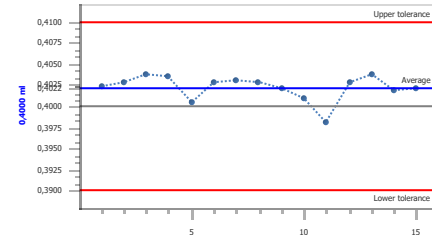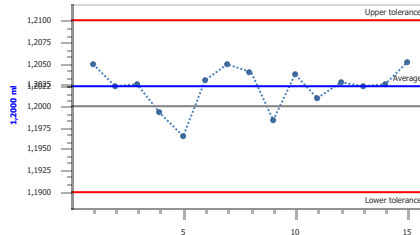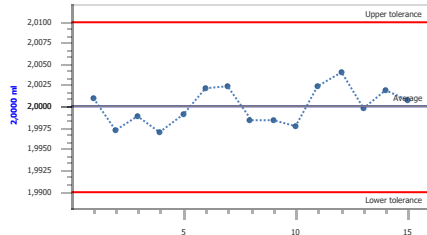

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 835

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:

7

Date:

28.11.2023

Balance:

Sartorius -
LE244S-OCE

DE-M