

# Certificate of performance



ISO 9001  
CERTIFIED

**Article:** 3 515 505

**Grad. pipette, 5:0,05 ml, AS, conf. cert.**




**Batch:** 25-22

**Serial:**

**Measuring Nr.** 56711

**Batch size:** 500

| Volume:         | 5,0000 ml   | 3,0000 ml   | 1,0000 ml   |
|-----------------|-------------|-------------|-------------|
| Tolerance:      | ± 0,0300 ml | ± 0,0300 ml | ± 0,0300 ml |
| Average value:  | 5,0039 ml   | 3,0033 ml   | 1,0053 ml   |
| Deviation:      | 0,0063 ml   | 0,0039 ml   | 0,0023 ml   |
| Precision (CV): | 0,1256 %    | 0,1291 %    | 0,2294 %    |

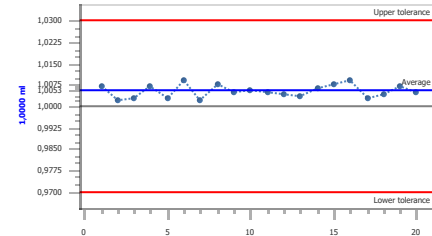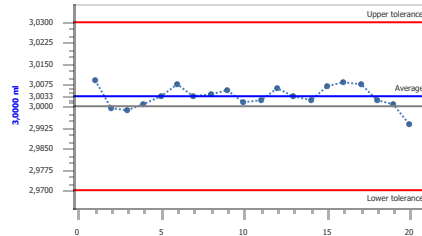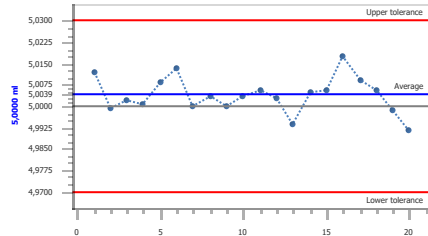

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 835

**witeg Labortechnik GmbH**

Am Bildacker 16  
97877 Wertheim  
Germany  
+49 (0) 9342 / 9301-0  
info@witeg.de

|           |                           |
|-----------|---------------------------|
| Operator: | 7                         |
| Date:     | 22.06.2022                |
| Balance:  | Sartorius -<br>LE244S-OCE |

DE-M