

Certificate of performance



Article: 3 515 505

Grad. pipette, 5:0,05 ml, AS, conf. cert.




Batch: 33-24

Serial:

Measuring Nr. 68867

Batch size: 800

Volume:	5,0000 ml	3,0000 ml	1,0000 ml
Tolerance:	± 0,0300 ml	± 0,0300 ml	± 0,0300 ml
Average value:	4,9919 ml	2,9963 ml	1,0018 ml
Deviation:	0,0088 ml	0,0067 ml	0,0037 ml
Precision (CV):	0,1763 %	0,2217 %	0,3704 %

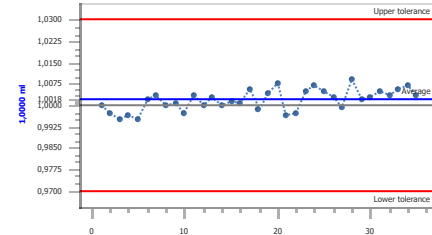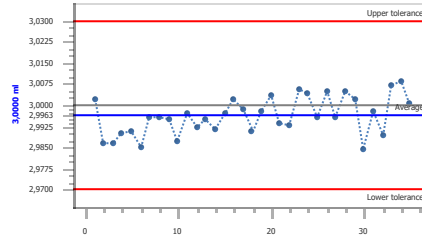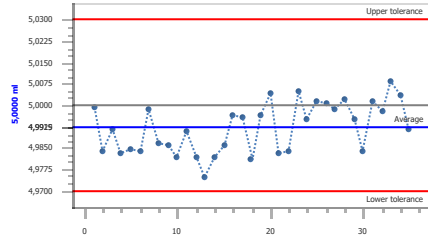

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 835

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	7
Date:	27.08.2024
Balance:	Sartorius - LE244S-OCE

