

# Certificate of performance



**Article:** 3 515 510

**Grad. pipettes, 5:0,1 ml, AS, conf. cert.**




**Batch:** 20-21

**Serial:**

**Measuring Nr.:** 47177

**Batch size:** 280

Volume:	5,0000 ml	3,0000 ml	1,0000 ml
<b>Tolerance:</b>	± 0,0300 ml	± 0,0300 ml	± 0,0300 ml
<b>Average value:</b>	4,9958 ml	2,9952 ml	0,9984 ml
<b>Deviation:</b>	0,0063 ml	0,0048 ml	0,0029 ml
<b>Precision (CV):</b>	0,1255 %	0,1595 %	0,2934 %

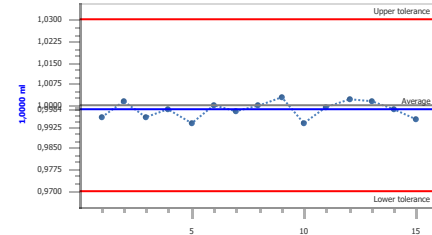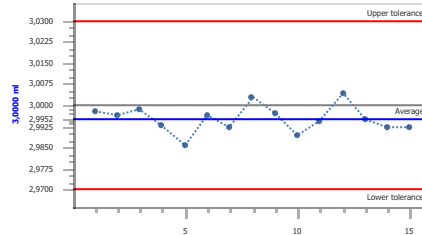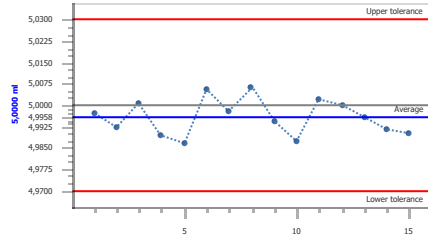

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 835

**witeg Labortechnik GmbH**

Am Bildacker 16  
97877 Wertheim  
Germany  
+49 (0) 9342 / 9301-0  
info@witeg.de

<b>Operator:</b>	7
<b>Date:</b>	08.06.2021
<b>Balance:</b>	Sartorius - LE244S-OCE

