

# Certificate of performance



ISO 9001  
CERTIFIED

**Article:** 3 515 510

**Grad. pipettes, 5:0,1 ml, AS, conf. cert.**




**Batch:** 09-23

**Serial:**

**Measuring Nr.** 61897

**Batch size:** 280

| Volume:                | 5,0000 ml   | 3,0000 ml   | 1,0000 ml   |
|------------------------|-------------|-------------|-------------|
| <b>Tolerance:</b>      | ± 0,0300 ml | ± 0,0300 ml | ± 0,0300 ml |
| <b>Average value:</b>  | 4,9866 ml   | 2,9893 ml   | 0,9988 ml   |
| <b>Deviation:</b>      | 0,0065 ml   | 0,0052 ml   | 0,0025 ml   |
| <b>Precision (CV):</b> | 0,1293 %    | 0,1721 %    | 0,2466 %    |

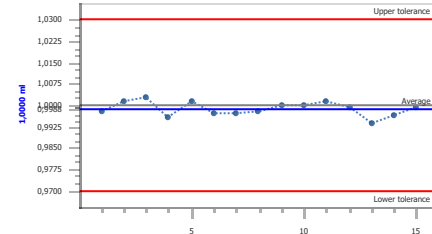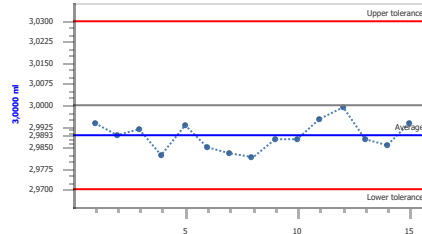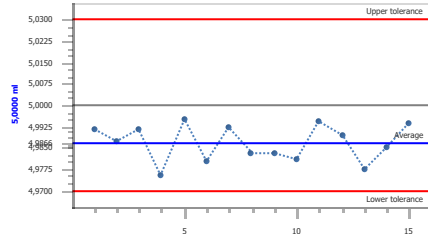

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 835

**witeg Labortechnik GmbH**

Am Bildacker 16  
97877 Wertheim  
Germany  
+49 (0) 9342 / 9301-0  
info@witeg.de

|                  |                           |
|------------------|---------------------------|
| <b>Operator:</b> | 7                         |
| <b>Date:</b>     | 08.03.2023                |
| <b>Balance:</b>  | Sartorius -<br>LE244S-OCE |

