

# Certificate of performance



ISO 9001  
CERTIFIED

**Article:** 3 515 810

**Grad. pipettes, 20:0,1 ml, AS, conf. cert.**




**Batch:** 06-22

**Serial:**

**Measuring Nr.** 52043

**Batch size:** 150

Volume:	20,000 ml	12,000 ml	4,000 ml
<b>Tolerance:</b>	± 0,1000 ml	± 0,1000 ml	± 0,1000 ml
<b>Average value:</b>	20,0251 ml	12,0175 ml	4,0080 ml
<b>Deviation:</b>	0,0223 ml	0,0128 ml	0,0076 ml
<b>Precision (CV):</b>	0,1115 %	0,1066 %	0,1902 %

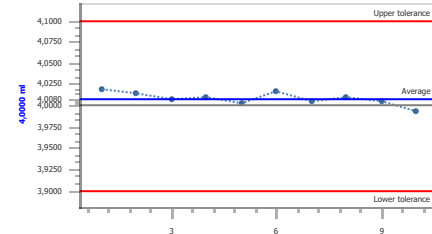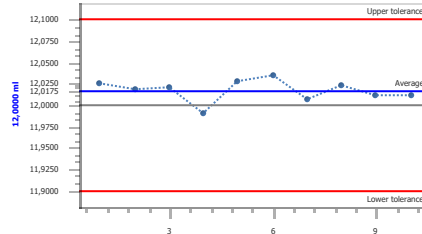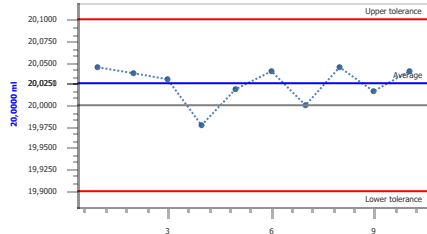

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 835

**witeg Labortechnik GmbH**

Am Bildacker 16  
97877 Wertheim  
Germany  
+49 (0) 9342 / 9301-0  
info@witeg.de

<b>Operator:</b>	7
<b>Date:</b>	09.02.2022
<b>Balance:</b>	Sartorius - LE244S-OCE

DE-M