

# Certificate of performance



ISO 9001  
CERTIFIED

**Article:** 3 517 011

**Enzyme test pipette, 0,1:0,001, AS, conf. cert.**

**Batch:** 19-19




**Serial:**

**Measuring Nr.** 30307

**Batch size:**

736

Volume:	0,1000 ml	0,0600 ml	0,0200 ml
Tolerance:	± 0,0030 ml	± 0,0030 ml	± 0,0030 ml
Average value:	0,0990 ml	0,0586 ml	0,0180 ml
Deviation:	0,0008 ml	0,0006 ml	0,0004 ml
Precision (CV):	0,7556 %	0,9791 %	1,8345 %

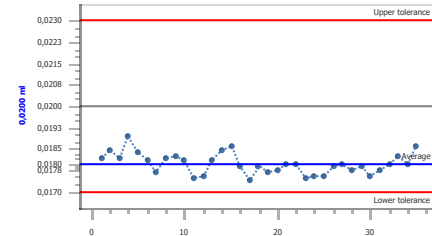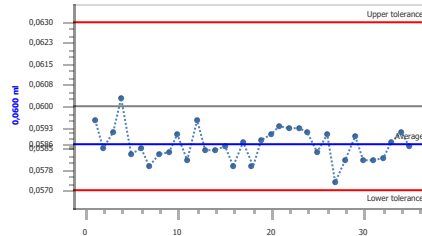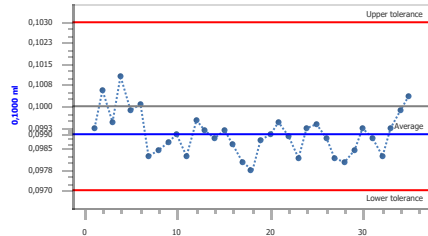

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to DIN 12699

**witeg Labortechnik GmbH**

Am Bildacker 16  
97877 Wertheim  
Germany  
+49 (0) 9342 / 9301-0  
info@witeg.de

Operator:	9
Date:	06.06.2019
Balance:	Sartorius - LE244S-0CE

