

# Certificate of performance



ISO 9001  
CERTIFIED

**Article:** 3 517 011

**Pipette f.encym.analysis., 0,1:0,001 ml, AS, conf. cert.**




**Batch:** 31-22

**Serial:**

**Measuring Nr.** 57782

**Batch size:** 265

Volume:	0,1000 ml	0,0600 ml	0,0200 ml
<b>Tolerance:</b>	± 0,0030 ml	± 0,0030 ml	± 0,0030 ml
<b>Average value:</b>	0,0999 ml	0,0600 ml	0,0188 ml
<b>Deviation:</b>	0,0008 ml	0,0006 ml	0,0007 ml
<b>Precision (CV):</b>	0,8463 %	1,0651 %	3,3007 %

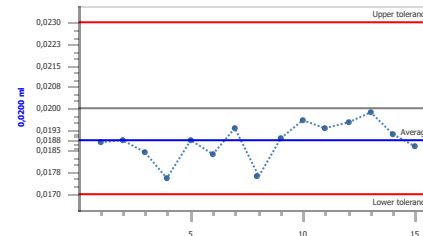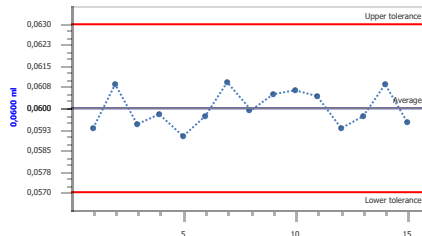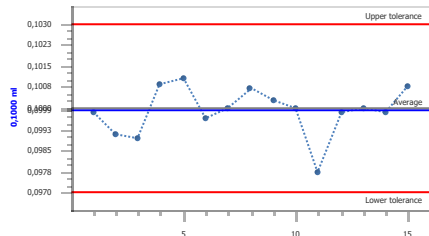

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to DIN 12699

**witeg Labortechnik GmbH**

Am Bildacker 16  
97877 Wertheim  
Germany  
+49 (0) 9342 / 9301-0  
info@witeg.de

<b>Operator:</b>	7
<b>Date:</b>	02.08.2022
<b>Balance:</b>	Sartorius - LE244S-OCE

