

# Certificate of performance



**Article:** 3 517 051

**Pipettes f. encym. analysis, 0,5:0,01 ml, AS, conf. cert.**




**Batch:** 10-20

**Serial:**

**Measuring Nr.** 36659

**Batch size:** 189

Volume:	0,5000 ml	0,3000 ml	0,1000 ml
<b>Tolerance:</b>	± 0,0050 ml	± 0,0050 ml	± 0,0050 ml
<b>Average value:</b>	0,4989 ml	0,2985 ml	0,0991 ml
<b>Deviation:</b>	0,0011 ml	0,0012 ml	0,0009 ml
<b>Precision (CV):</b>	0,2113 %	0,3838 %	0,9396 %

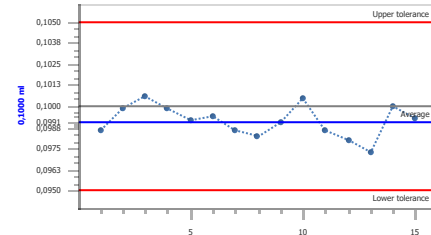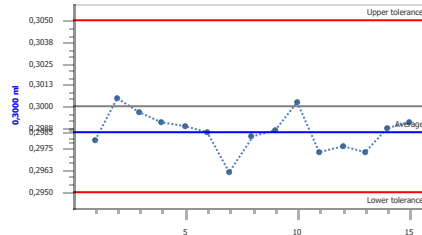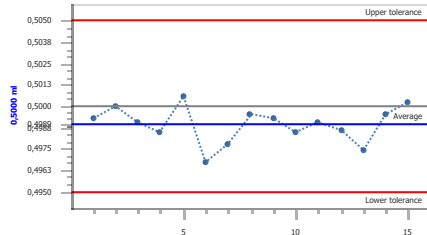

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to DIN 12 699

**witeg Labortechnik GmbH**

Am Bildacker 16  
97877 Wertheim  
Germany  
+49 (0) 9342 / 9301-0  
info@witeg.de

<b>Operator:</b>	9
<b>Date:</b>	13.03.2020
<b>Balance:</b>	Sartorius - LE244S-OCE

