

# Certificate of performance



**Article:** 3 517 051

**Pipettes f. encym. analysis, 0,5:0,01 ml, AS, conf. cert.**




**Batch:** 38-21

**Serial:**

**Measuring Nr.** 49475

**Batch size:** 227

Volume:	0,5000 ml	0,3000 ml	0,1000 ml
<b>Tolerance:</b>	± 0,0050 ml	± 0,0050 ml	± 0,0050 ml
<b>Average value:</b>	0,4987 ml	0,2998 ml	0,0996 ml
<b>Deviation:</b>	0,0015 ml	0,0016 ml	0,0005 ml
<b>Precision (CV):</b>	0,3066 %	0,5338 %	0,5190 %

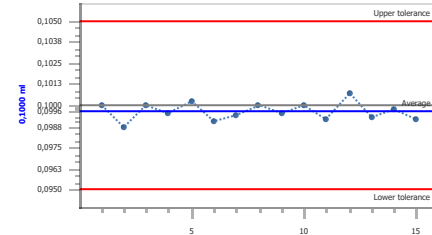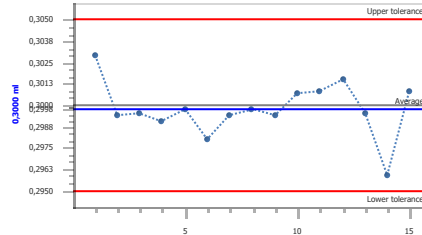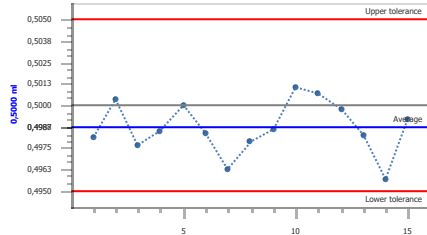

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to DIN 12 699

**witeg Labortechnik GmbH**

Am Bildacker 16  
97877 Wertheim  
Germany  
+49 (0) 9342 / 9301-0  
info@witeg.de

<b>Operator:</b>	7
<b>Date:</b>	01.10.2021
<b>Balance:</b>	Sartorius - LE244S-OCE

