

# Certificate of performance



**Article:** 3 517 710

**Pipettes f. encym. analysis, 10:0,1 ml, AS, conf. cert.**




**Batch:** 25-22

**Serial:**

**Measuring Nr.** 56608

**Batch size:** 499

| Volume:                | 10,000 ml   | 6,0000 ml   | 2,0000 ml   |
|------------------------|-------------|-------------|-------------|
| <b>Tolerance:</b>      | ± 0,0500 ml | ± 0,0500 ml | ± 0,0500 ml |
| <b>Average value:</b>  | 10,0100 ml  | 6,0079 ml   | 2,0104 ml   |
| <b>Deviation:</b>      | 0,0111 ml   | 0,0059 ml   | 0,0042 ml   |
| <b>Precision (CV):</b> | 0,1111 %    | 0,0978 %    | 0,2093 %    |

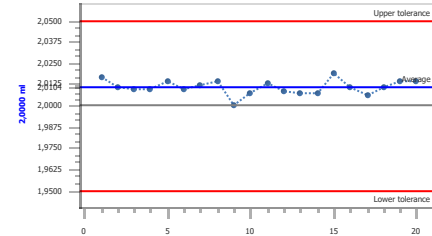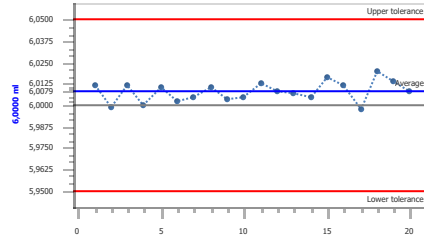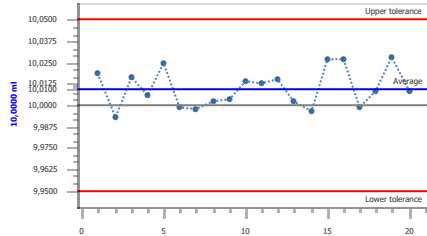

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to DIN 12699

**witeg Labortechnik GmbH**

Am Bildacker 16  
97877 Wertheim  
Germany  
+49 (0) 9342 / 9301-0  
info@witeg.de

|                  |                           |
|------------------|---------------------------|
| <b>Operator:</b> | 7                         |
| <b>Date:</b>     | 20.06.2022                |
| <b>Balance:</b>  | Sartorius -<br>LE244S-OCE |

