

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 535 030

Volumetric pipettes, 3 ml, AS, conf. cert.

Batch: 31-22


Serial:

Measuring Nr. 57825

Batch size:

1200

| | |
|------------------------|------------------|
| Volume: | 3,0000 ml |
| Tolerance: | $\pm 0,0100$ ml |
| Average value: | 2,9997 ml |
| Deviation: | 0,0020 ml |
| Precision (CV): | 0,0661 % |

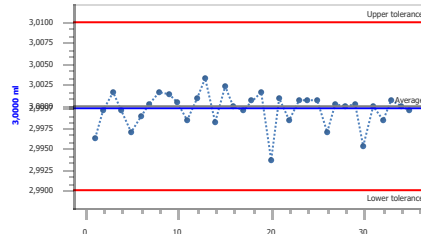

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 648

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:

7

Date:

05.08.2022

Balance:

Sartorius -
LE244S-OCE

DE-M