

# Certificate of performance



ISO 9001  
CERTIFIED

**Article:** 3 535 090

**Volumetric pipettes, 9 ml, AS, conf. cert.**

**Batch:** 39-22


**Serial:**

**Measuring Nr.** 59935

**Batch size:**

252

|                        |                  |
|------------------------|------------------|
| <b>Volume:</b>         | <b>9,0000 ml</b> |
| <b>Tolerance:</b>      | $\pm 0,0200$ ml  |
| <b>Average value:</b>  | 9,0030 ml        |
| <b>Deviation:</b>      | 0,0026 ml        |
| <b>Precision (CV):</b> | 0,0293 %         |

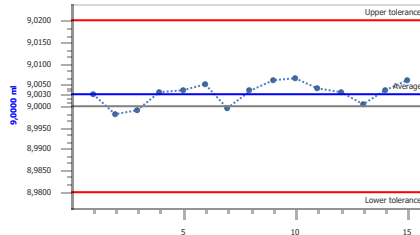

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 648

**witeg Labortechnik GmbH**

Am Bildacker 16  
97877 Wertheim  
Germany  
+49 (0) 9342 / 9301-0  
info@witeg.de

**Operator:**

4

**Date:**

27.10.2022

**Balance:**

Sartorius -  
MSE224S-0CE  
-DU

DE-M