

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 535 100 USP

Volumetric pipettes, 10 ml, AS, USP, conf. cert.


Batch: 50-23

Serial:

Measuring Nr. 65739

Batch size: 277

| | |
|------------------------|-------------------|
| Volume: | 10,0000 ml |
| Tolerance: | $\pm 0,0200$ ml |
| Average value: | 10,0005 ml |
| Deviation: | 0,0027 ml |
| Precision (CV): | 0,0270 % |

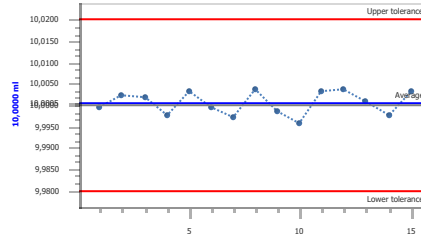

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 648

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

| | |
|------------------|---------------------------|
| Operator: | 7 |
| Date: | 16.01.2024 |
| Balance: | Sartorius - LE244S-OCE |

DE-M