

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 535 120 USP

Volumetric pipettes, 12 ml, USP, AS, conf. cert.


Batch: 22-20

Serial:

Measuring Nr. 38466

Batch size: 59

Volume:	12,0000 ml
Tolerance:	$\pm 0,0200$ ml
Average value:	11,9965 ml
Deviation:	0,0040 ml
Precision (CV):	0,0332 %

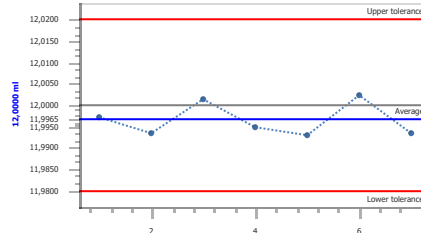

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 648

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	7
Date:	08.06.2020
Balance:	Sartorius - MSE224S-0CE -DU

DE-M