

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 535 200

Volumetric pipettes, 20 ml, AS, conf. cert.


Batch: 07-24

Serial:

Measuring Nr. 65996

Batch size: 497

| | |
|------------------------|-----------------|
| Volume: | 20,000 ml |
| Tolerance: | $\pm 0,0300$ ml |
| Average value: | 20,0014 ml |
| Deviation: | 0,0074 ml |
| Precision (CV): | 0,0369 % |

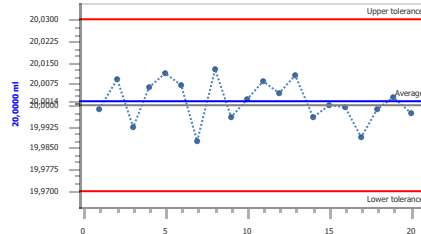

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 648

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator: 7

Date: 12.02.2024

Balance: Sartorius -
LE244S-OCE

DE-M