

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 535 500

Volumetric pipettes, 50 ml, AS, conf. cert.

Batch: 12-20


Serial:

Measuring Nr. 37670

Batch size:

1197

Volume:	50,0000 ml
Tolerance:	$\pm 0,0500$ ml
Average value:	50,0055 ml
Deviation:	0,0139 ml
Precision (CV):	0,0278 %

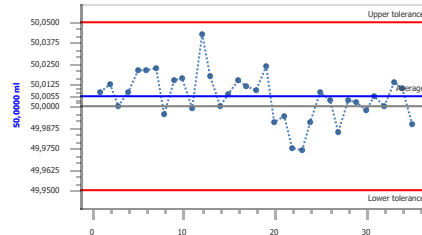

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 648

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:

7

Date:

04.05.2020

Balance:

Sartorius -
MSE224S-0CE
-DU

DE-M