

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 555 010

Volumetric pipettes, 1 ml, 2 marks, AS, conf. cert.


Batch: 14-22

Serial:

Measuring Nr. 55143

Batch size: 1186

Volume:	1,0000 ml
Tolerance:	$\pm 0,0080$ ml
Average value:	1,0000 ml
Deviation:	0,0016 ml
Precision (CV):	0,1587 %

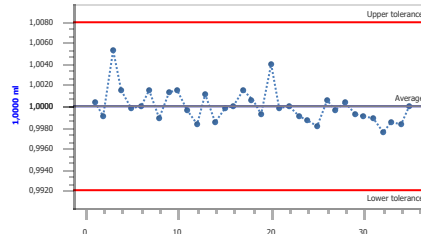

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 648

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	4
Date:	03.05.2022
Balance:	Sartorius - MSE224S-0CE -DU

DE-M