

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 555 025

Volumetric pipettes, 2,5 ml, 2 marks, AS, conf. cert.

Batch: 07-21


Serial:

Measuring Nr. 44990

Batch size:

150

Volume:	2,5000 ml
Tolerance:	$\pm 0,0100$ ml
Average value:	2,4980 ml
Deviation:	0,0028 ml
Precision (CV):	0,1138 %

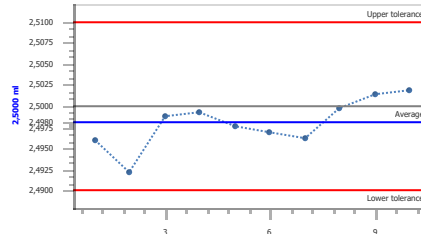

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 648

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:

7

Date:

09.03.2021

Balance:

Sartorius -
LE244S-OCE

DE-M