

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 555 090

Volumetric pipettes, 9 ml, with 2 marks, AS, conf. cert.


Batch: 41-18

Serial:

Measuring Nr. 25392

Batch size: 90

Volume:	9,0000 ml
Tolerance:	$\pm 0,0200$ ml
Average value:	8,9996 ml
Deviation:	0,0029 ml
Precision (CV):	0,0322 %

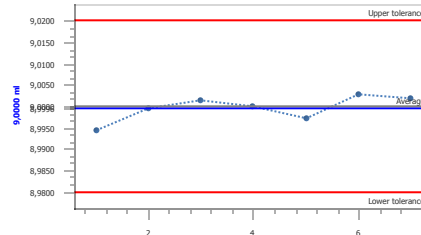

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 648

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	4
Date:	06.11.2018
Balance:	Sartorius - LE244S-OCE

DE-M