

# Certificate of performance



ISO 9001  
CERTIFIED

**Article:** 3 010 253 B

**Burettes, 25 ml, str. stopc., amber grad., AS, conf. cert.**




**Batch:** 47-15

**Serial:**

**Measuring Nr.:** 49942

**Batch size:** 100

Volume:	25,0000 ml	15,0000 ml	5,0000 ml
<b>Tolerance:</b>	± 0,0300 ml	± 0,0300 ml	± 0,0300 ml
<b>Average value:</b>	25,0061 ml	15,0024 ml	5,0078 ml
<b>Deviation:</b>	0,0066 ml	0,0075 ml	0,0040 ml
<b>Precision (CV):</b>	0,0265 %	0,0502 %	0,0802 %

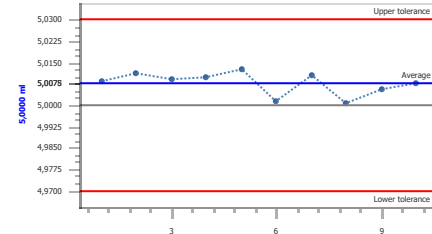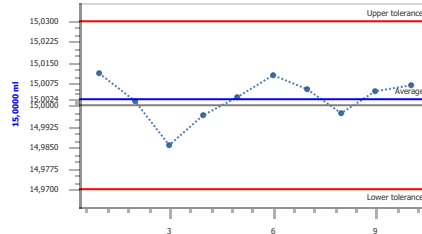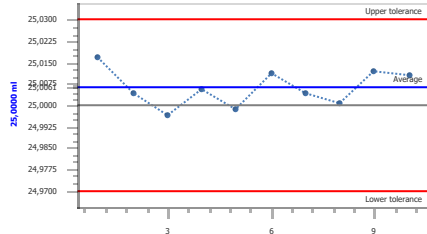

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

**witeg Labortechnik GmbH**

Am Bildacker 16  
97877 Wertheim  
Germany  
+49 (0) 9342 / 9301-0  
info@witeg.de

<b>Operator:</b>	7
<b>Date:</b>	25.10.2021
<b>Balance:</b>	Sartorius - LE244S-OCE

