

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 122 105

Pellet-burettes, 10 ml, lat. needle valve, AS, conf. cert.




Batch: 09-21

Serial:

Measuring Nr.: 58251

Batch size: 10

Volume:	10,0000 ml	6,0000 ml	2,0000 ml
Tolerance:	± 0,0200 ml	± 0,0200 ml	± 0,0200 ml
Average value:	9,9968 ml	5,9952 ml	2,0095 ml
Deviation:	0,0066 ml	0,0055 ml	0,0050 ml
Precision (CV):	0,0662 %	0,0923 %	0,2484 %

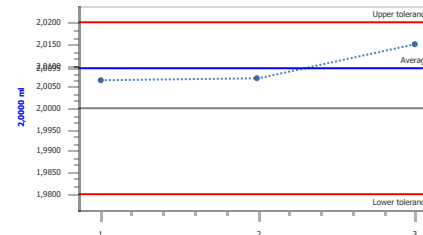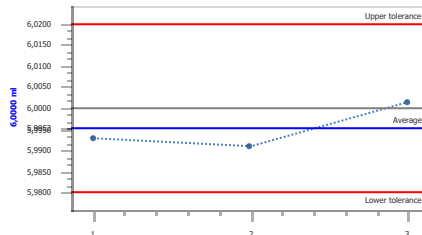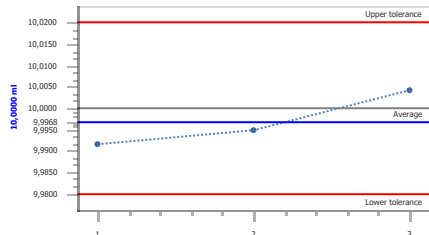

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	7
Date:	23.08.2022
Balance:	Sartorius - LE244S-OCE

