

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 124 255

Pellet-burettes, 25 ml, amber glass, AS, conf.cert.




Batch: 44-21

Serial:

Measuring Nr.: 52773

Batch size: 22

Volume:	25,0000 ml	15,0000 ml	5,0000 ml
Tolerance:	± 0,0300 ml	± 0,0300 ml	± 0,3000 ml
Average value:	25,0027 ml	14,9990 ml	5,0061 ml
Deviation:	0,0080 ml	0,0119 ml	0,0038 ml
Precision (CV):	0,0321 %	0,0791 %	0,0754 %

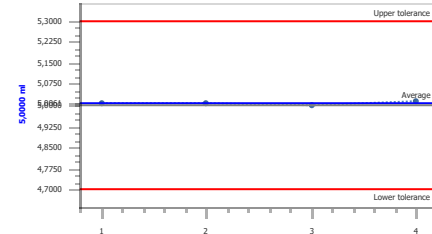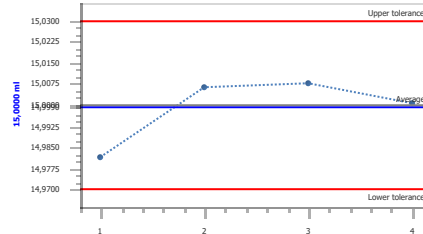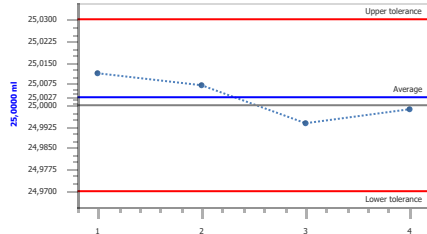

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	7
Date:	03.03.2022
Balance:	Sartorius - LE244S-OCE

