

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 715 003

Graduated cylinder, 25:0,5 ml, A, conf. cert




Batch: 30-24

Serial:

Measuring Nr. 68272

Batch size: 500

| Volume: | 5,0000 ml | 15,0000 ml | 25,0000 ml |
|-----------------|-------------|-------------|-------------|
| Tolerance: | ± 0,2500 ml | ± 0,2500 ml | ± 0,2500 ml |
| Average value: | 4,9777 ml | 15,0063 ml | 25,0213 ml |
| Deviation: | 0,0395 ml | 0,0427 ml | 0,0512 ml |
| Precision (CV): | 0,7907 % | 0,2846 % | 0,2048 % |

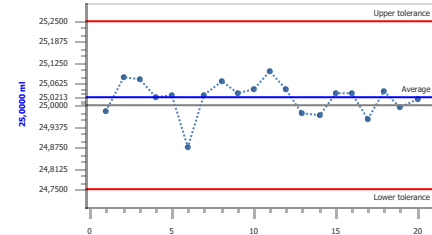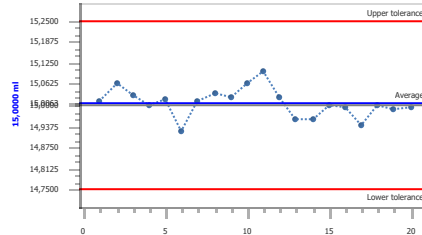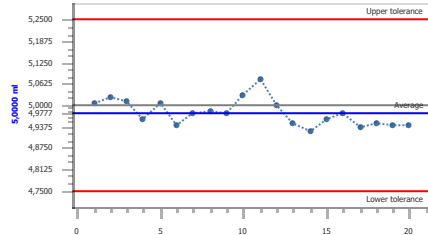

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 4788

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

| | |
|-----------|-----------------------------------|
| Operator: | 4 |
| Date: | 31.07.2024 |
| Balance: | Sartorius - MSE224S-0CE -DU |

