

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 715 025 USP

Graduated cylinders, 250:2 ml, A, USP, conf. cert.




Batch: 34-24

Serial:

Measuring Nr. 68866

Batch size: 248

Volume:	50,0000 ml	150,0000 ml	250,0000 ml
Tolerance:	± 1,0000 ml	± 1,0000 ml	± 1,0000 ml
Average value:	49,8133 ml	149,9603 ml	250,1304 ml
Deviation:	0,2232 ml	0,2020 ml	0,1932 ml
Precision (CV):	0,4463 %	0,1347 %	0,0773 %

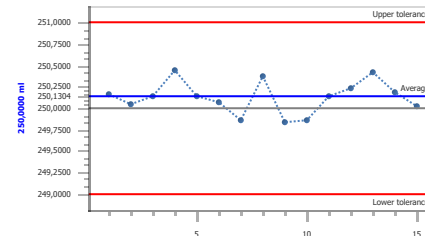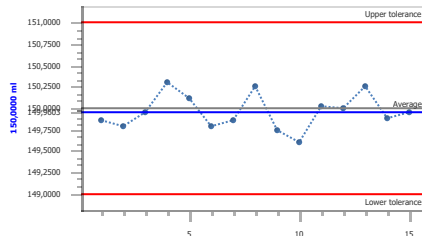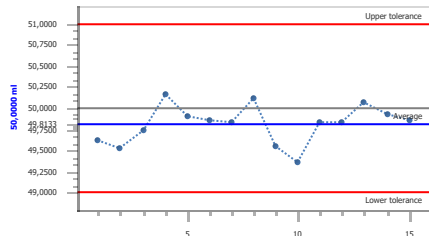

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 4788

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	4
Date:	26.08.2024
Balance:	Sartorius - LA 1200 S

